


ŀ

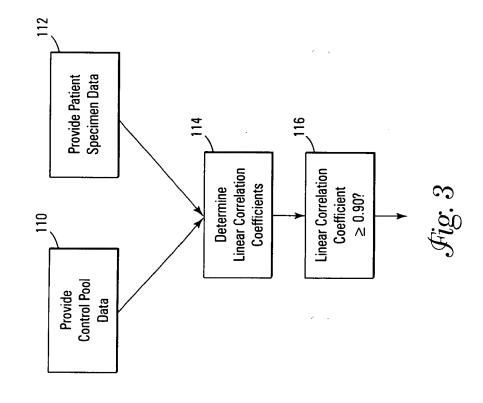

CLICAL ASSAY CALIBRATION ADJUSTMENT METHOD George G. Klee 09/853,867

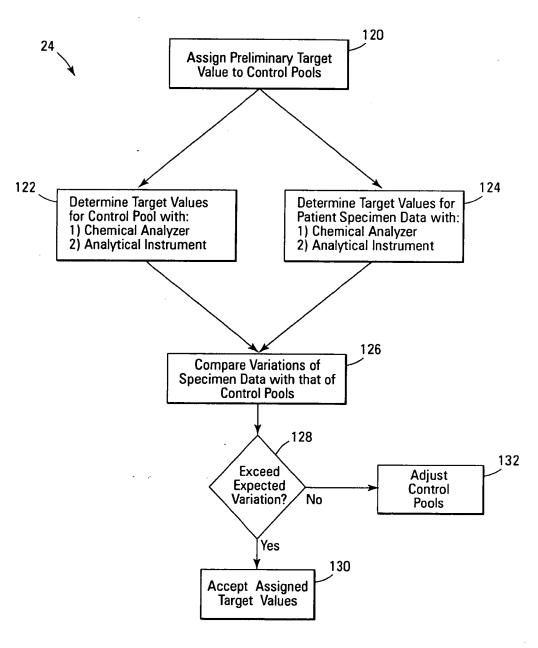
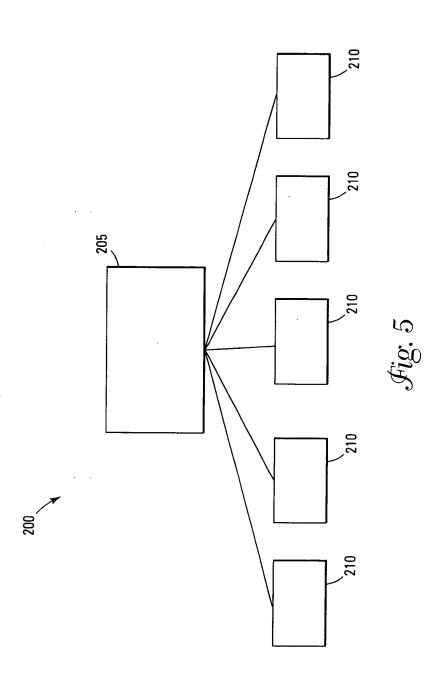
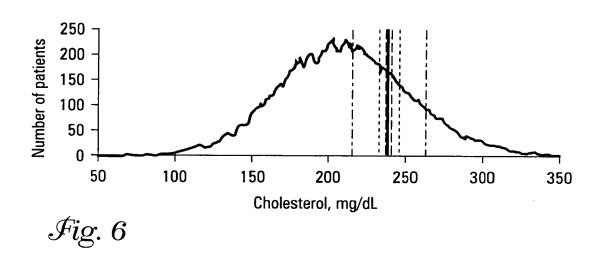
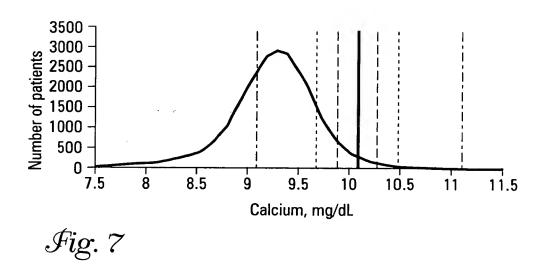
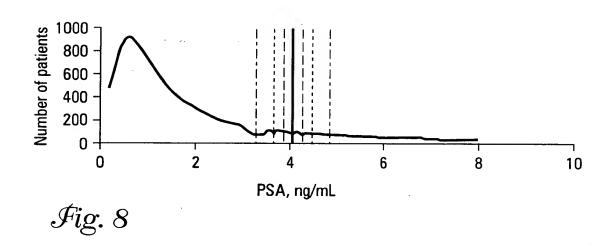



Fig. 4










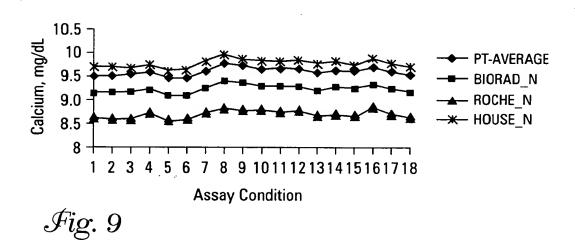

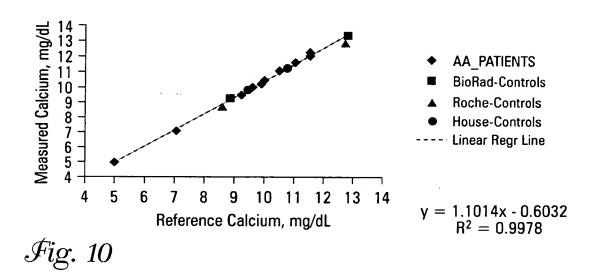

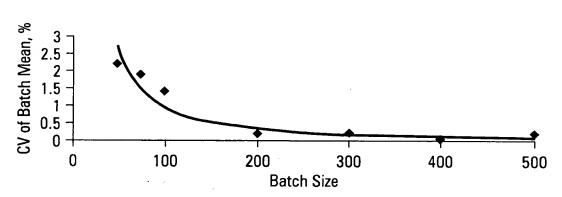


Fig. 11

